


Tumark[®] Conic

REF

351260

351262

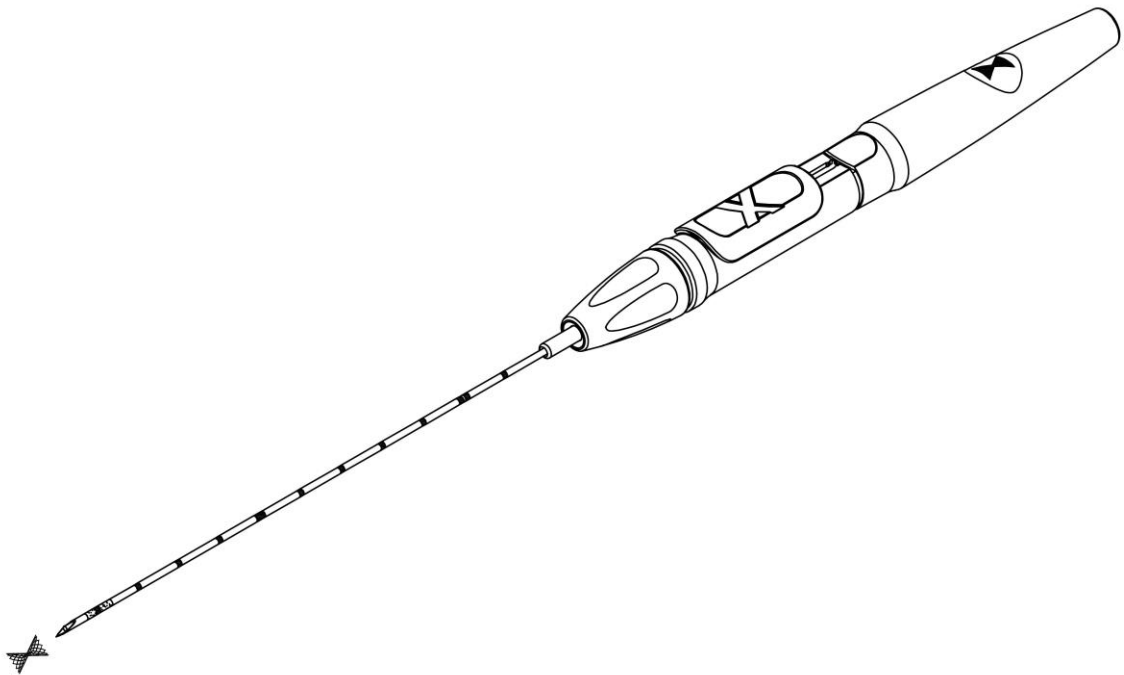

INSTRUCTIONS FOR USE OF THE DEVICE IN THE USA

HOLOGIC[®]

INSTRUCTIONS FOR USE**Read instructions before use****Keep for future reference****Important Information:**

Read this instruction manual thoroughly and be familiar with its contents prior to use. Failure to read the entire manual and to familiarize yourself with all instructions before using the *Tumark® Conic* is unsafe and can result in life threatening or severe injury to the patient or user and in damage or malfunction of the device.

Indications:

The *Tumark® Conic* is intended to attach a marker to soft breast tissue and axillary lymph nodes, following an open or a percutaneous procedure to radiographically mark the location of the surgical site. It is not indicated to be used with magnetic resonance imaging (MRI) techniques.

Contraindications:

- The *Tumark® Conic* is not intended for use except as indicated above.
- The use of the *Tumark® Conic* system is contraindicated in patients who suffer from a severe nickel allergy.

Duration of use:

The clip marker of the *Tumark® Conic* is a permanent implant (> 30 days).

Warnings:

- Only qualified physicians with knowledge, experience and training in percutaneous soft tissue marking shall use the *Tumark® Conic*.
- This manual does not include descriptions or instructions for surgical techniques. It is the responsibility of the physician performing any procedure to determine the appropriateness of the procedure to be performed and of the use of this device and to determine the specific technique for each patient.
- DO NOT use the system in patients with breast implants.
- The *Tumark® Conic* should only be used if the indicator on the packaging is green, only before the expiration date, and only if the packaging is unopened and undamaged. Product sterility can only be guaranteed if these criteria are met. If the indicator is not green, if the expiration date is exceeded, or if the packaging is damaged or opened before use, the product should not be used and the distributor or manufacturer, SOMATEX, should be contacted.
- The product is intended for single use only: DO NOT reuse or resterilize.
- When using a positioning needle, the *Tumark® Conic* must be checked for compatibility in advance. The beveled *Tumark® Conic* cannula tip opening should protrude fully out of the positioning needle and the user should be able to gauge this protrusion in order to be able to apply the clip marker safely and not place it too far into the tissue.
- Care must be taken, when marking axillary lymph nodes in particular, NOT to trap nearby blood vessels with the clip marker and not to damage a nearby nerve.
- If the clip marker, which was placed in the area of the axillary lymph nodes, cannot be found again, it is important to identify and ensure its location.
- When marking axillary lymph nodes there is a potential risk of introducing the clip marker into the venous system and embolizing downstream.

Precautions:

- The *Tumark® Conic* clip marker is made from a nickel-titanium alloy (Nitinol), which is why the product is contraindicated in patients with severe nickel allergy.
- Make sure that the slide button remains in the retracted position while the cannula is being put in position.
- The clip marker must be placed by pushing the slide button forward as far as possible to the stop position.
- There is risk of injury due to the sharp cannula tip. Use care especially when unpacking the cannula.
- The cannula of *Tumark® Conic* is NOT made of MRI-compatible metals. NOT suitable for MRI safety area. Danger of injury!
- Pay attention to the dimensions of the clip marker in relation to the size of the tissue area being marked (see Product Description).
- In rare cases the expansion of the clip marker may be delayed. Visibility in radiological imaging might be compromised until full expansion.
- **Caution: Federal (USA) Law restricts this device to sale by or on the order of a physician.**

Information about materials used:

The implantable clip marker is made from a nickel-titanium alloy (Nitinol).

MRI Safety Information application system:

MR unsafe

The *Tumark® Conic* as an application system for clip markers is **not** suitable for use in MRI.

MRI Safety Information clip marker:

MR conditional

Clip markers, which have already been placed inside a patient, are conditionally MR safe. A patient with a clip marker can be safely scanned in an MR system meeting the following conditions:

- static magnetic field up to 3.0 Tesla with
- theoretically estimated maximum whole body averaged (WBA) specific absorption rate (SAR) of 2 W/kg.

Non-clinical tests were performed on the following systems:

- 1.5 Tesla Philips Achieva dStream (Philips Healthcare, Best, The Netherlands) MRI with software 5.4.1\5.4.1.2
- 3 Tesla Philips Ingenia (Philips Healthcare, Best, The Netherlands) MRI with software 5.3.1\5.3.1.3

Under the scanning conditions defined above, it is expected that clip marker of *Tumark® Conic* will produce the following maximum RF-related temperature rise:

- at 1.5 Tesla: < 1,0 °C (2 W/kg SAR) after 20 min of continuous scanning,
- at 3.0 Tesla: < 1,0 °C (2 W/kg SAR) after 20 min of continuous scanning.


Under the scanning conditions defined above, it is expected that clip marker of *Tumark® Conic* will produce the following image artefacts:

- at 1.5 Tesla: 2.0 mm spin echo sequence; 2.7 mm gradient echo sequence;
- at 3.0 Tesla: 3.8 mm spin echo sequence; 4.5 mm gradient echo sequence.


Do not expose the implanted clip marker to unconventional and non-standardized MRI techniques other than the ones listed above, because it has NOT BEEN TESTED for that purpose.

Product Description:

This is a sterile product for single use only and consists of a non-absorbable nickel-titanium clip marker (1), an introducer cannula (2) and a plastic handle. When new and unopened, the clip marker is contained within the cannula. The cannula tip is beveled to help insertion, has markings 1 cm apart for measuring the depth of penetration, and a textured surface behind the cannula tip. The handle is equipped with a slide button (3) which allows one handed placement of the marker by pressing it forward. A safety catch system prevents the slide button from inadvertently moving forward and therefore prevents premature deployment of the marker. The clip marker has an hourglass shape. The symbol of the clip marker shape is depicted on the handle (4).



Schematic illustration

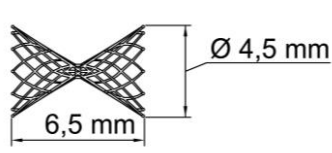

Dimensions of clip marker

Directions for Use:

1. Before opening, make sure that the packaging is not already open or damaged, that the indicator on the packaging is green, and that it is within the expiration date.
2. Disinfect the puncture area and cover the area around it with sterile drapes if required.
3. Use suitable imaging methods (ultrasound, mammography) to identify the target area. NOTE: the *Tumark® Conic* cannula is not suitable for the MRI safety zone.
4. Open the packaging and remove the product from packaging.
5. Remove the cannula protection hose from the outer cannula by twisting.
6. Use the cannula (2) to puncture the target area, and insert into the tissue. The depth of insertion can be read from the markings on the cannula when positioning the cannula tip.
7. Check the position of the cannula tip using suitable imaging techniques, and adjust if appropriate.
8. Place the clip marker (1) by pushing the slide button (3) forward as far as it will go.
9. Verify and record the position of the clip marker (1).
10. Remove the cannula (2).
11. Treat the wound.
12. After use: dispose the application device properly, following internal guidelines if appropriate; however, at least one suitable container intended for contaminated cannulas should be provided to ensure safe disposal.



















Warning:

We do not assume any liability for the use of this product or its components in case of re-sterilization or reuse. This product may not be reused after a single application. The quality of the materials, coats and adhesive joints could degrade. Safe use is not guaranteed any longer. The product that is already used once is not designed for the required cleaning and sterilization processes. The sterility of the reprocessed disposable products is therefore not guaranteed. The risk of unwanted injuries and infections, especially cross-infections between patient and medical staff inappropriately increases.

Storage Instructions:

Store in a dry and cool area at a temperature of 41 – 86 °F / 5 – 30 °C.
Keep away from sunlight and heat.

SYMBOLS

	Caution		Do not use if package is damaged
	Consult instructions for use		Single sterile barrier system with protective packaging outside
REF	Catalogue number		Single sterile barrier system
LOT	Batch code		Green indicator: Product is sterilized
	Date of manufacture		Temperature limit
	Manufacturer		Not made with natural rubber latex
	Expiration date		Keep away from sunlight and heat
STERILE EO	Sterilized by ethylene oxide		Store in a dry place
MD	Medical Device		MR unsafe (concerns only cannula)
	Do not reuse		MR conditional (concerns only clip marker)
	Do not resterilize	Rx ONLY	Caution: Federal (USA) Law restricts this device to sale by or on the order of a physician
L	Length		Diameter
UDI	Unique Device Identifier	QTY	Quantity

ORDERING

REF	Name	Diameter	Length
351260	Tumark® Conic	1.2 mm / 18 G	100 mm
351262	Tumark® Conic	1.2 mm / 18 G	120 mm

HOLOGIC[®] Distributed by:
Hologic, Inc.
250 Campus Drive
Marlborough, MA 01752 USA
Phone: 877-371-4372
email: mammosupport@hologic.com
www.hologic.com



SOMATEX Medical Technologies GmbH
Kaiserin-Augusta-Allee 112/113
10553 Berlin
Germany