

OPERATING ROOM

*FIBROIDS ≤ 5 CM and ALL POLYPS*

MyoSure®  
**XL**  
device

*FIBROIDS <3CM, RETAINED PRODUCTS  
OF CONCEPTION and ALL POLYPS*

MyoSure®  
**REACH**  
device

*DIRECTED BIOPSY and POLYPS ≤ 3 CM*

MyoSure®  
**LITE**  
device

*DIRECTED BIOPSY and POLYPS ≤ 1 CM*

MyoSure®  
**MANUAL**  
device

OUTPATIENT SETTING


## The MyoSure® suite FOR A FULL SPECTRUM OF INTRAUTERINE PROCEDURES

### Use the full capabilities of the MyoSure suite to:

- Perform a variety of procedures to help treat a wide range of intrauterine pathology
- Bring efficiency and consistency to your procedural choices
- Have the flexibility to perform procedures in any setting
- Achieve more complete resections and tissue collections



# SOLUTIONS FOR A WIDE RANGE OF PATHOLOGY

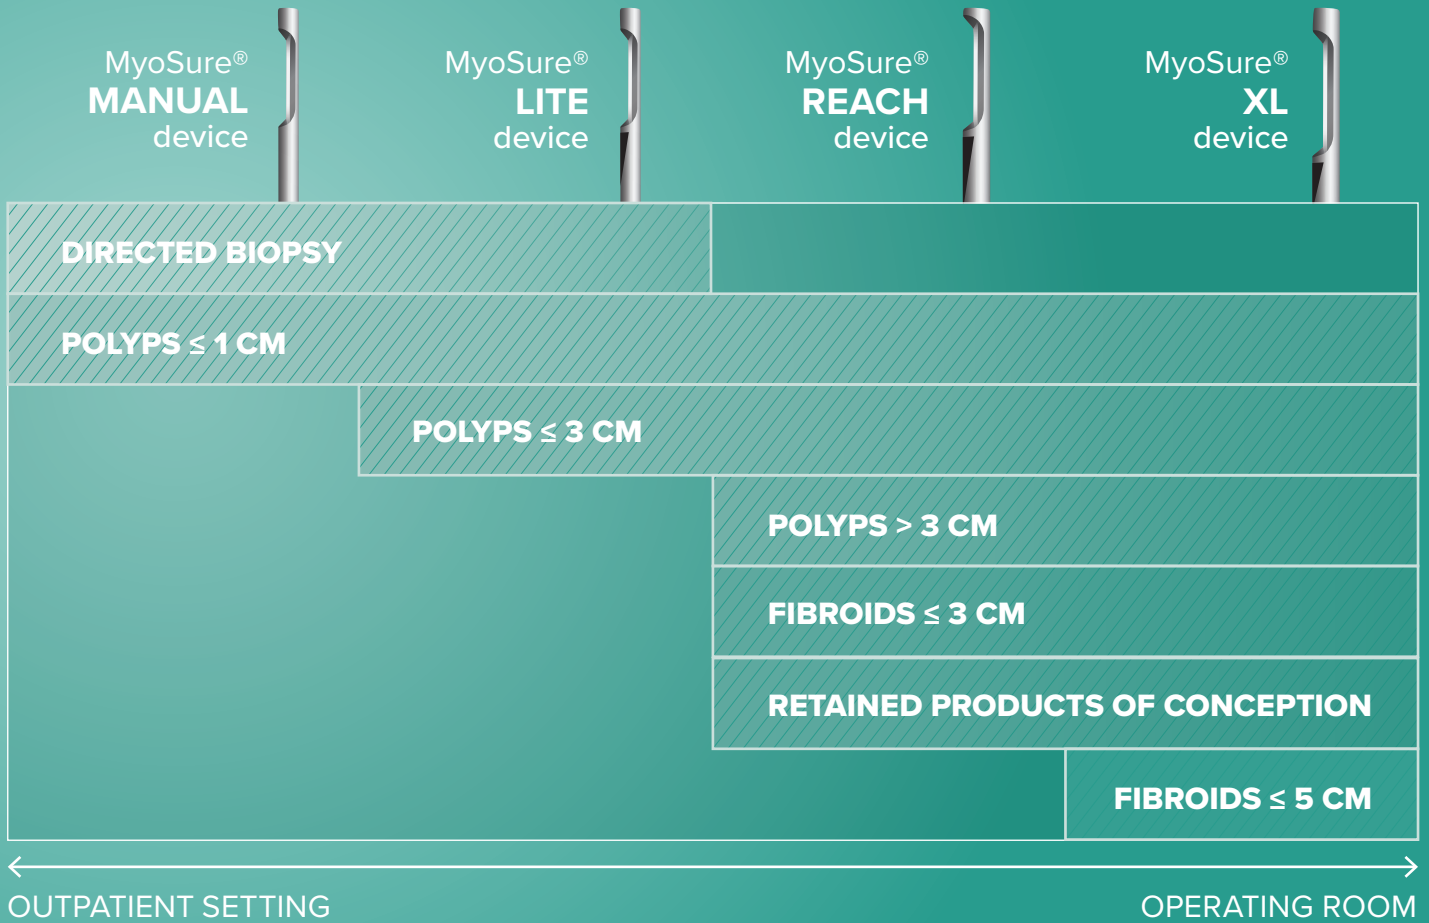

## Simplify the standard of care with the complete MyoSure® tissue removal suite

- Visualise procedures through the high-resolution, rod lens optics of the Omni® Hysteroscope
- Potentially save costs by using the right device for the right intrauterine procedure
- The Fluent® fluid management system is designed to optimise high aspiration procedures such as those performed with a MyoSure® tissue removal device\*

*Bring efficiency and consistency to your procedural choices—ask for a demo or visit [gynsurgicalsolutions.co.uk](https://gynsurgicalsolutions.co.uk) to learn more*



### IMPORTANT SAFETY INFORMATION

The MyoSure® tissue removal system, consisting of the MyoSure® tissue removal devices (LITE, REACH, XL) and MyoSure® controller, is intended for hysteroscopic intrauterine procedures by trained gynaecologists to resect and remove tissue, including submucous myomas, endometrial polyps and retained products of conception. The MyoSure® MANUAL tissue removal device is intended for hysteroscopic intrauterine procedures by trained gynaecologists to resect and remove tissue including focal lesions, such as endometrial polyps and retained products of conception. MyoSure® products are not appropriate for patients who are, or may be, pregnant, or are exhibiting pelvic infection, cervical malignancies, or previously diagnosed uterine cancer. For more details on risks and benefits of the MyoSure® system, MyoSure® MANUAL tissue removal device, Omni® Hysteroscope and the Fluent® fluid control system please see their respective IFUs.

\*The MyoSure® MANUAL device does not require an automated fluid management system, such as the Fluent® fluid Control system. Additionally, the MyoSure® MANUAL device does not require the MyoSure® controller unit.

Surgical Solutions | [Hologic.com](https://Hologic.com) | [euinfo@hologic.com](mailto:euinfo@hologic.com)

PB-00612-EUR-EN Rev 002 ©2021 Hologic, Omni, MyoSure and associated logos are trademarks or registered trademarks of Hologic, Inc. and/or its subsidiaries in the United States and/or other countries. This information is intended for medical professionals and is not intended as a product solicitation or promotion where such activities are prohibited. Because Hologic materials are distributed through websites, eBroadcasts and tradeshows, it is not always possible to control where such materials appear. For specific information on what products are available for sale in a particular country, please contact your local Hologic representative or write to [euinfo@hologic.com](mailto:euinfo@hologic.com)

**MyoSure®**  
Tissue Removal Simplified